



Image pickup unit 402
for binning number 2

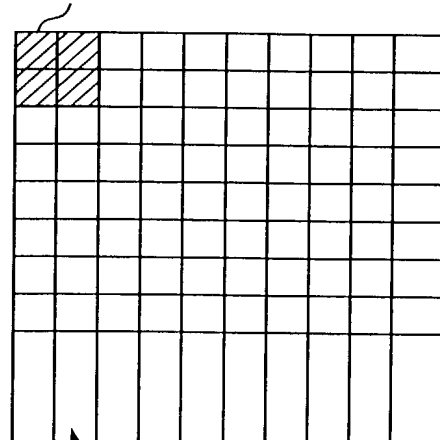
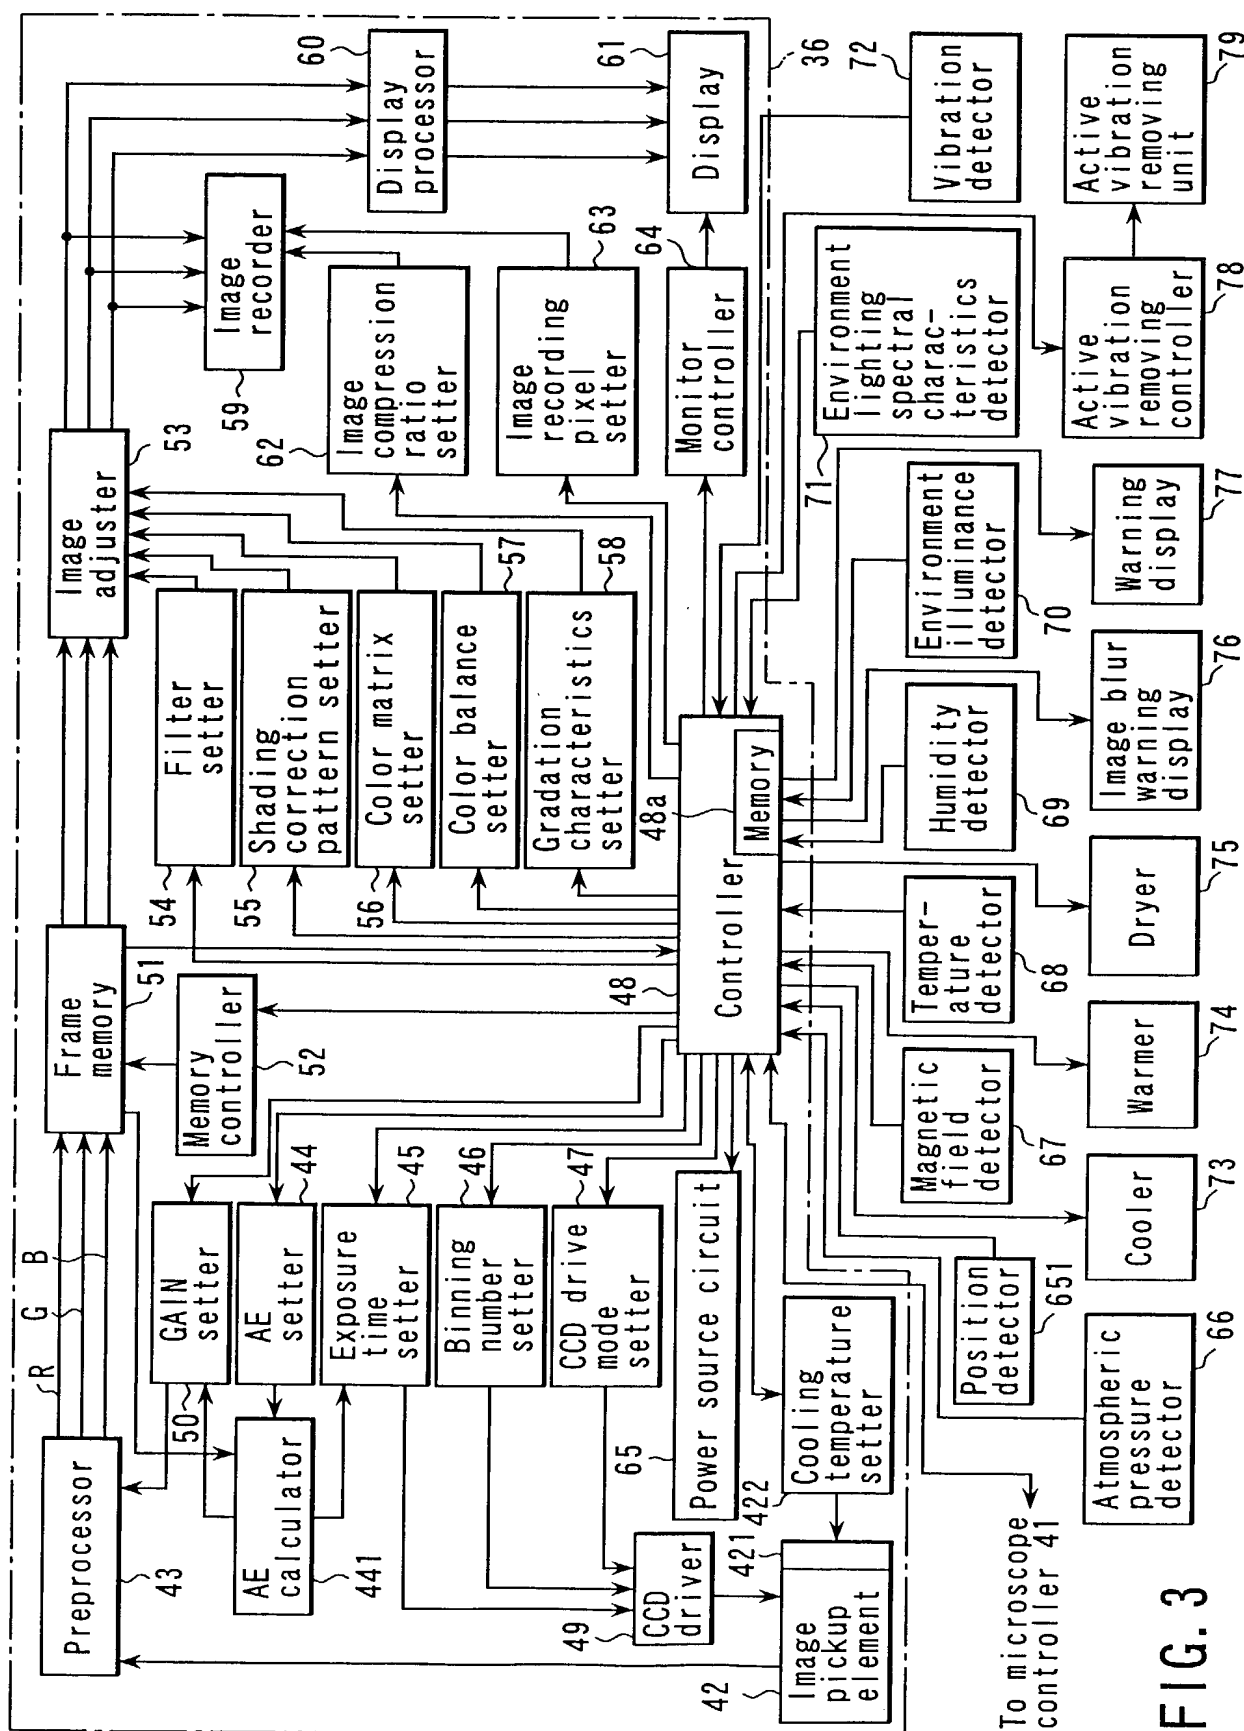


Image pickup
element 42

FIG. 4B



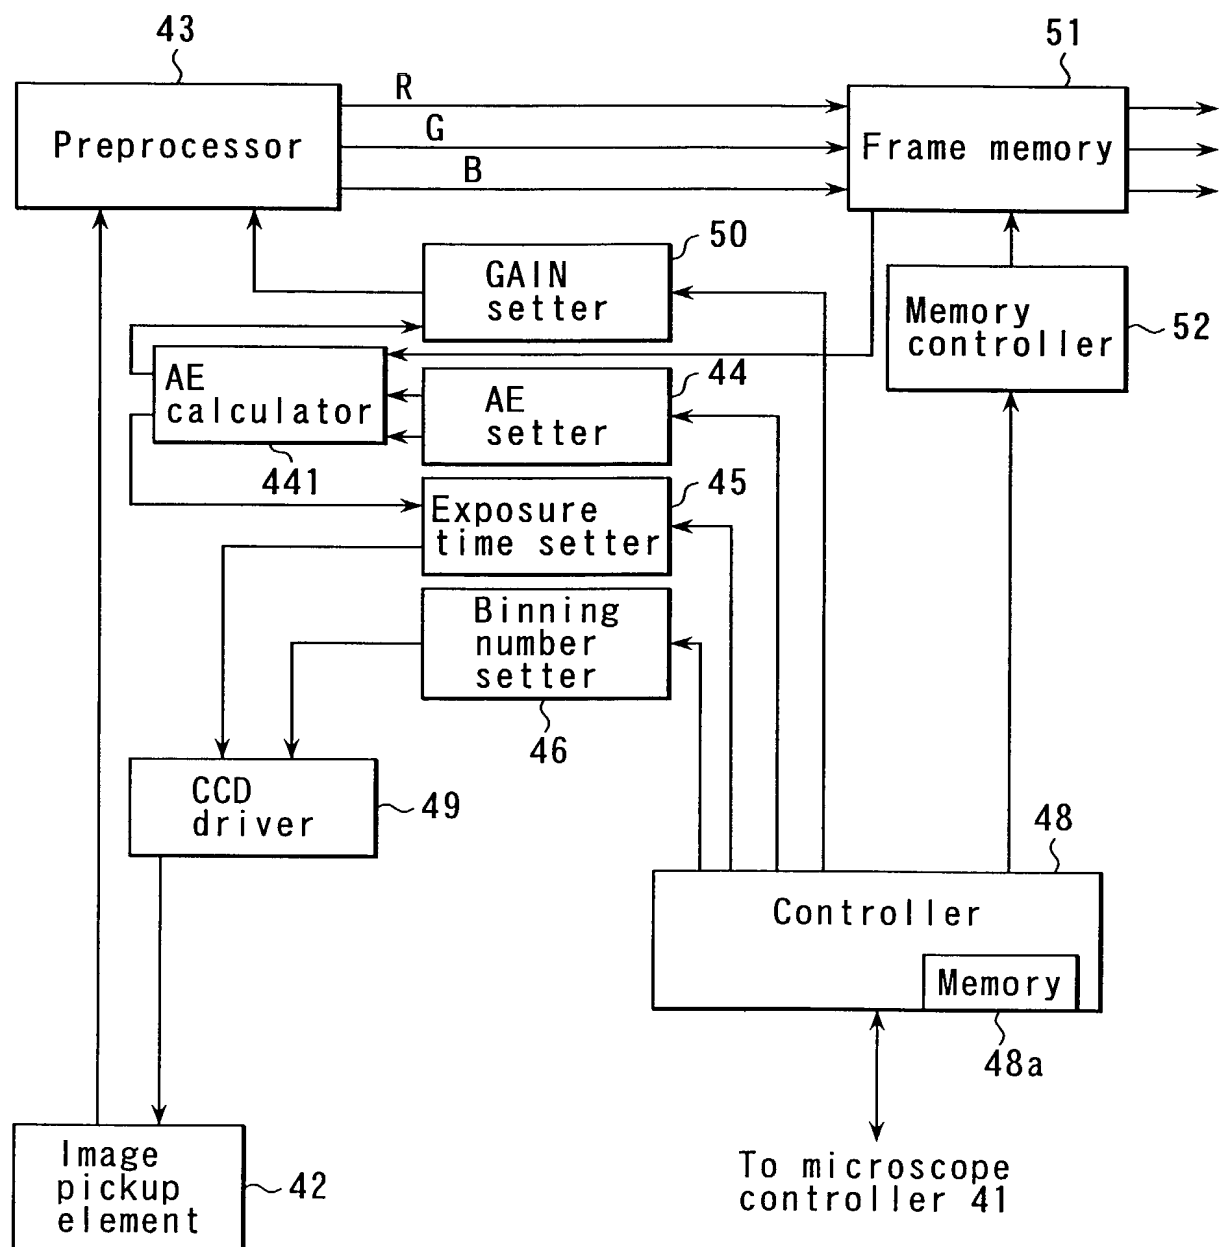


FIG. 5

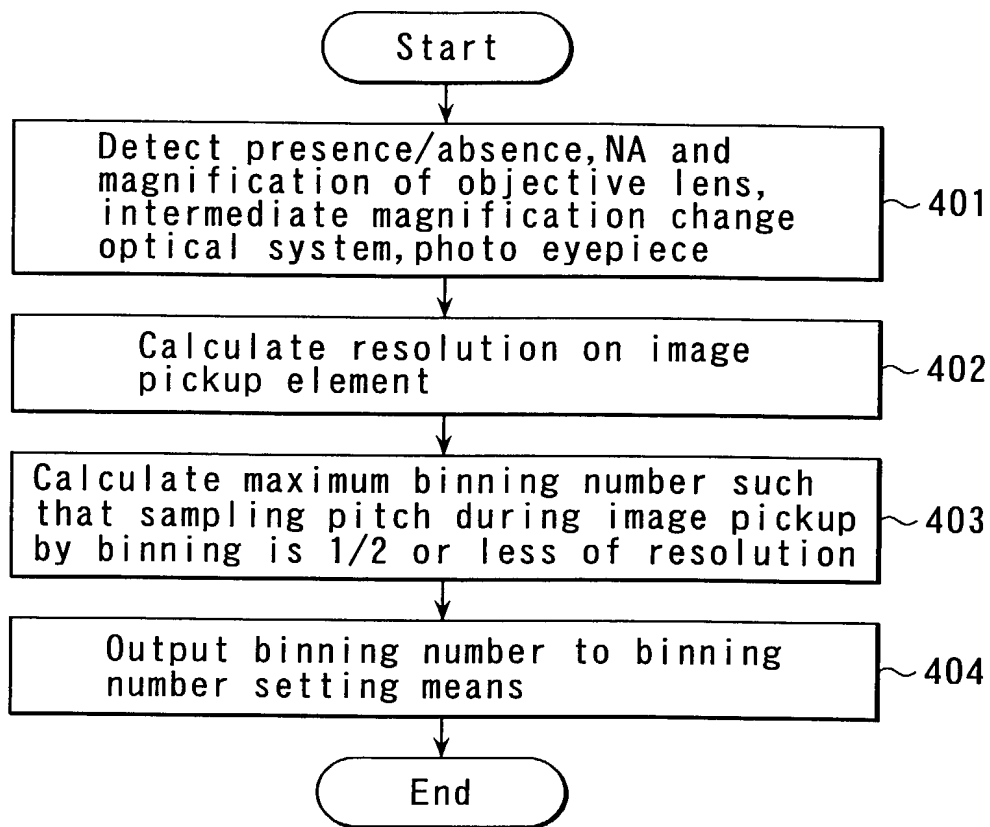


FIG. 6

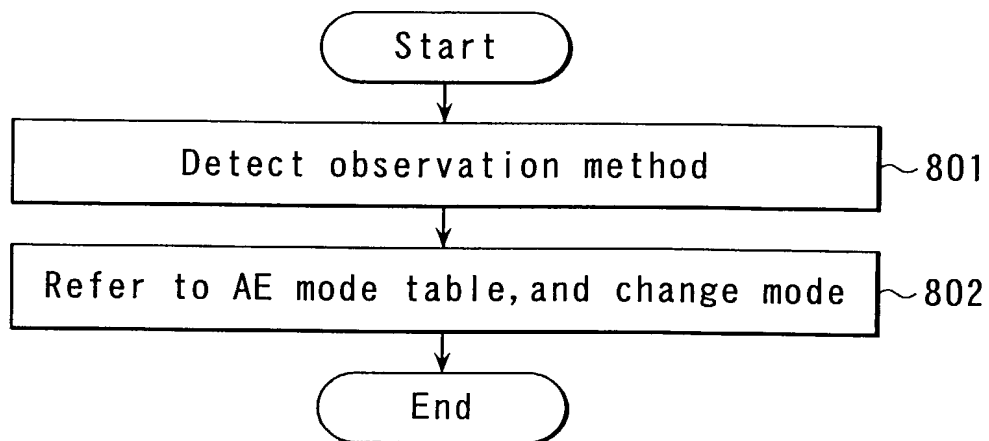


FIG. 7

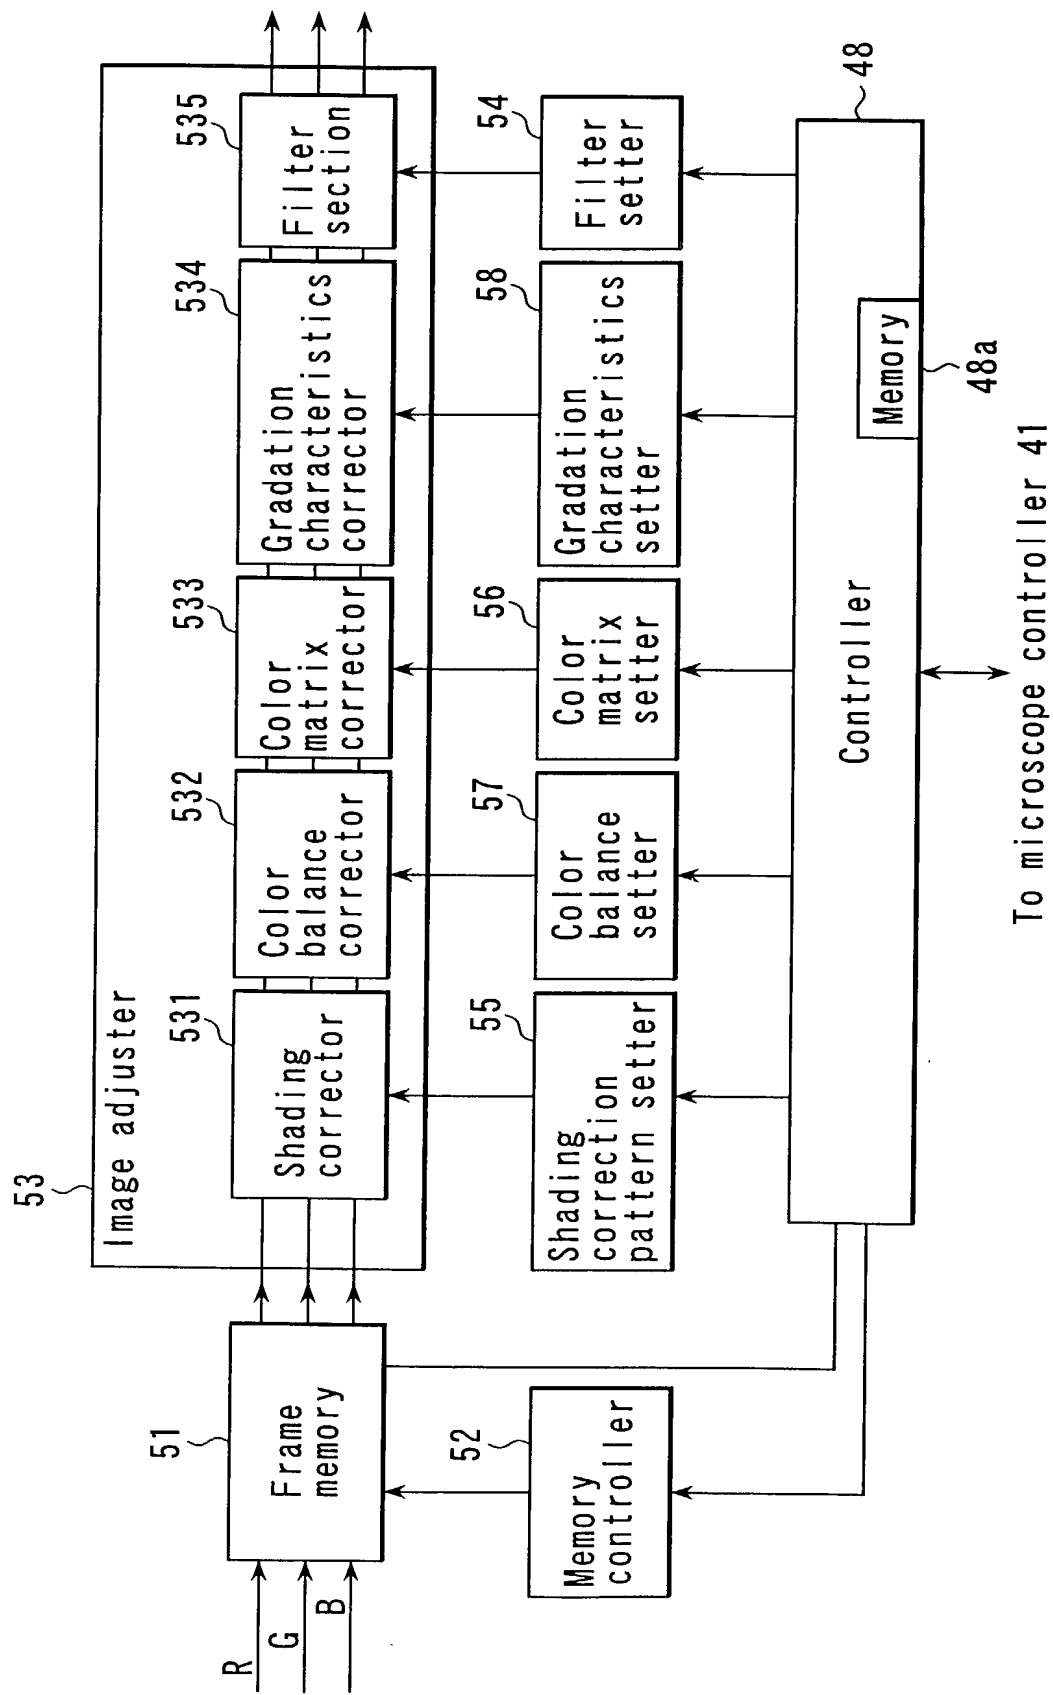


FIG. 8

To microscope controller 41

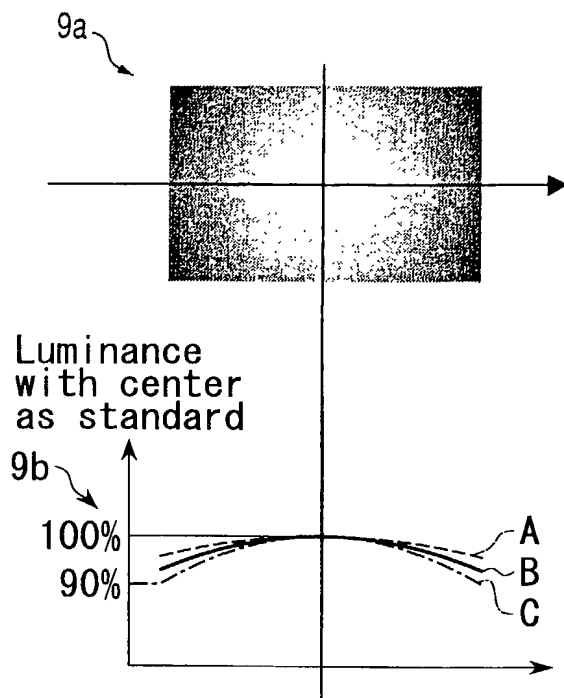


FIG. 9A

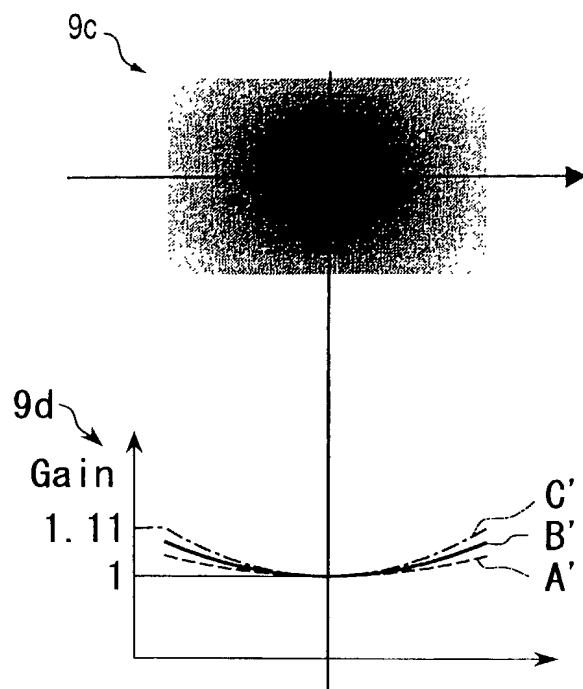


FIG. 9B

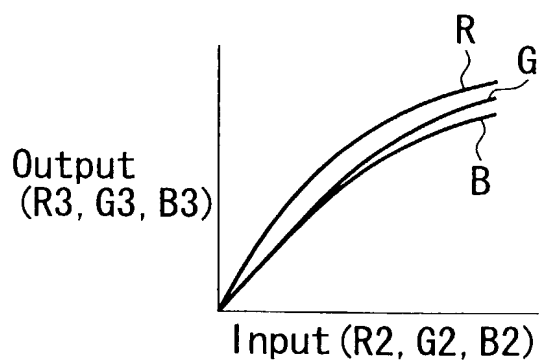


FIG. 10A

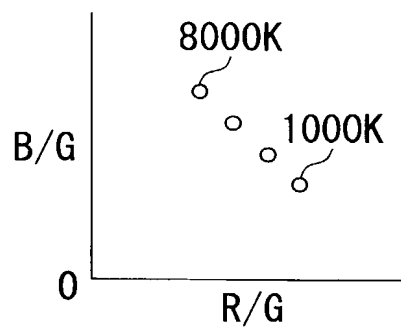


FIG. 10B

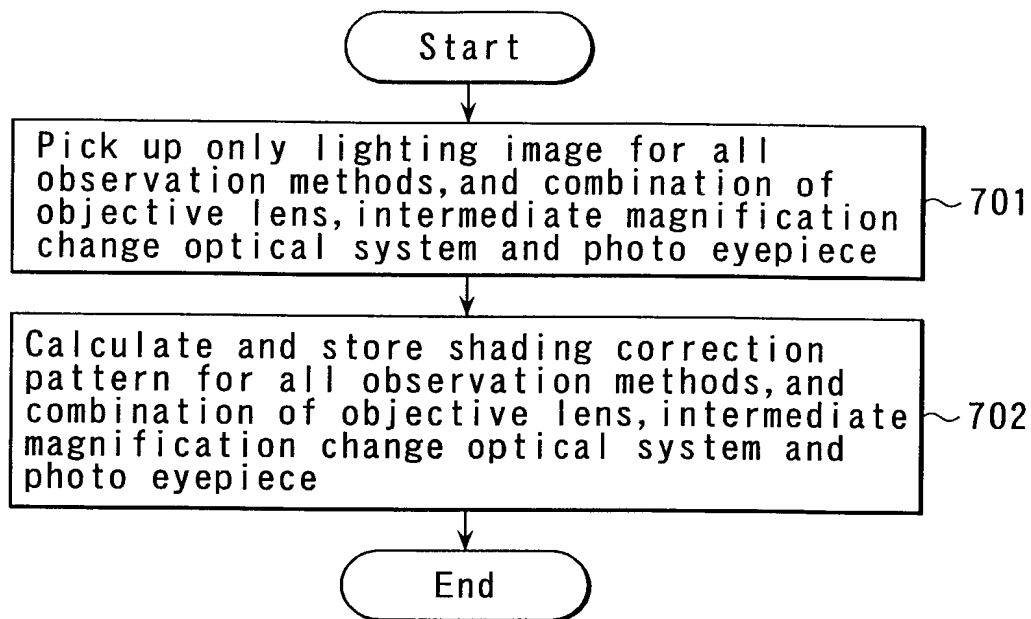


FIG. 11A

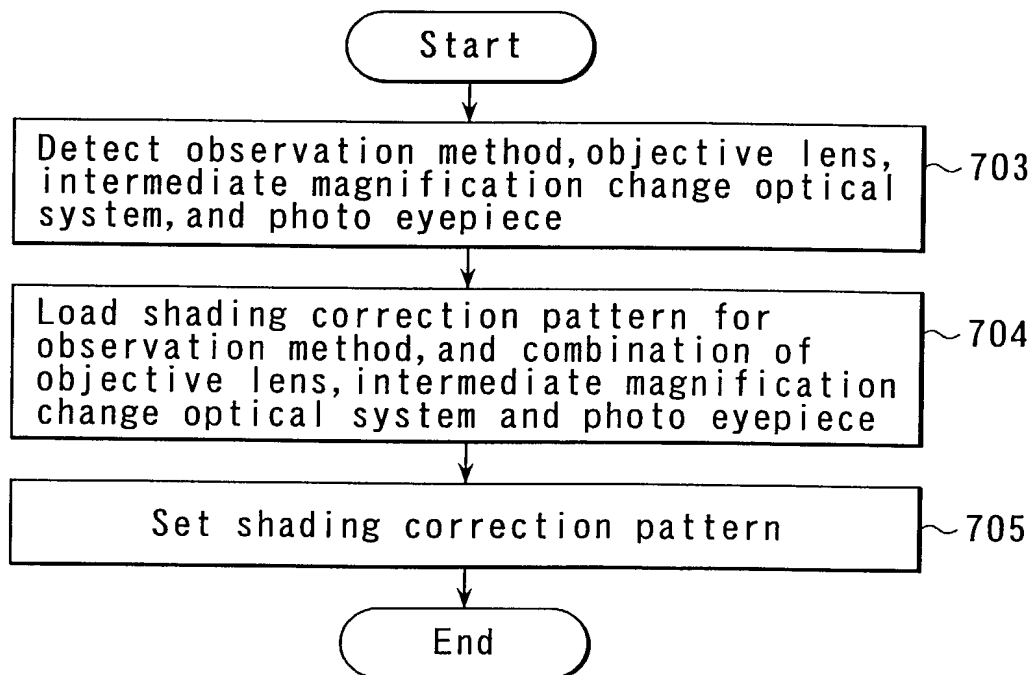


FIG. 11B

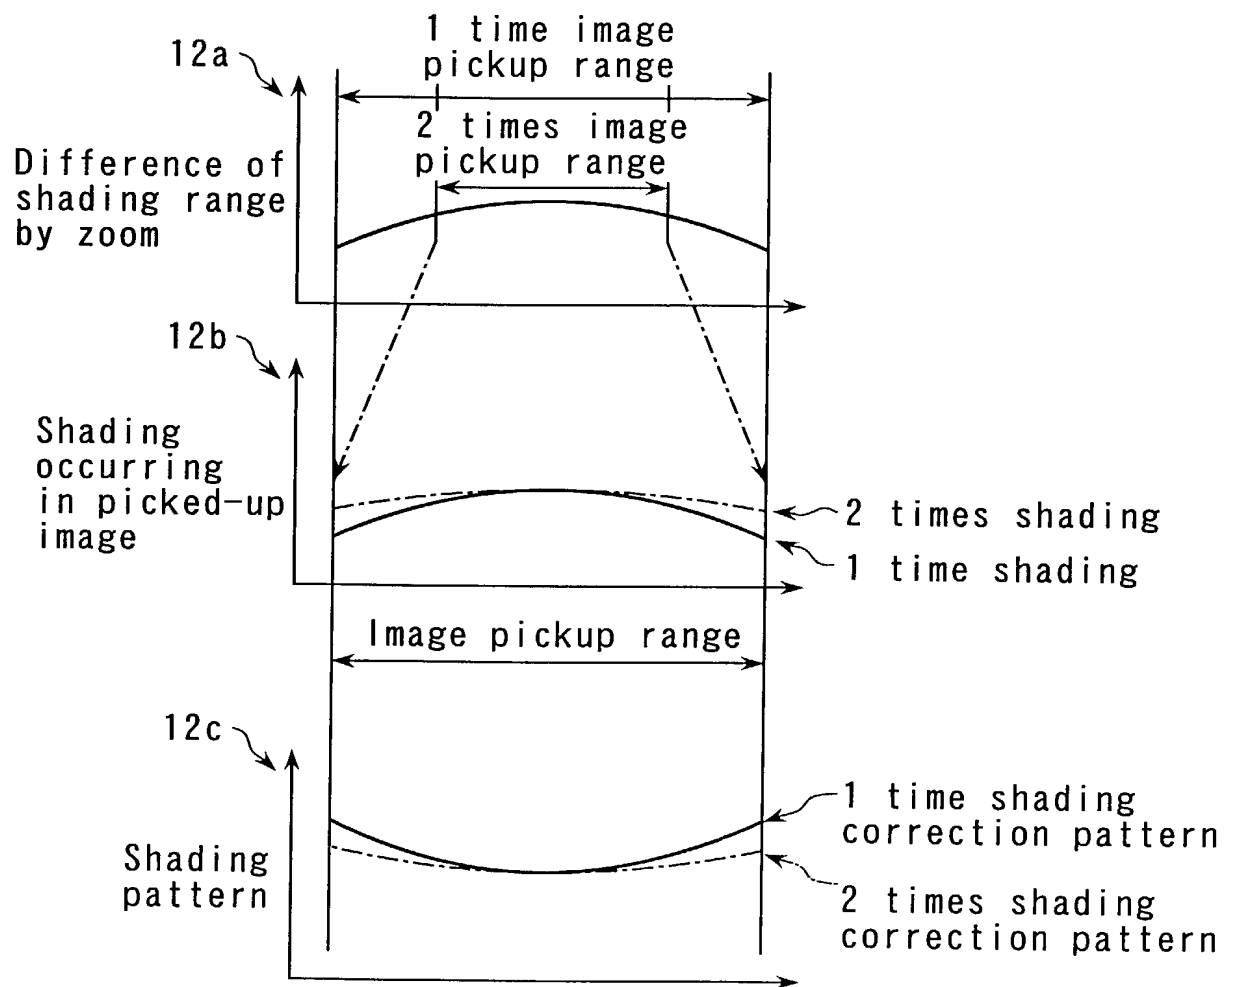


FIG. 12

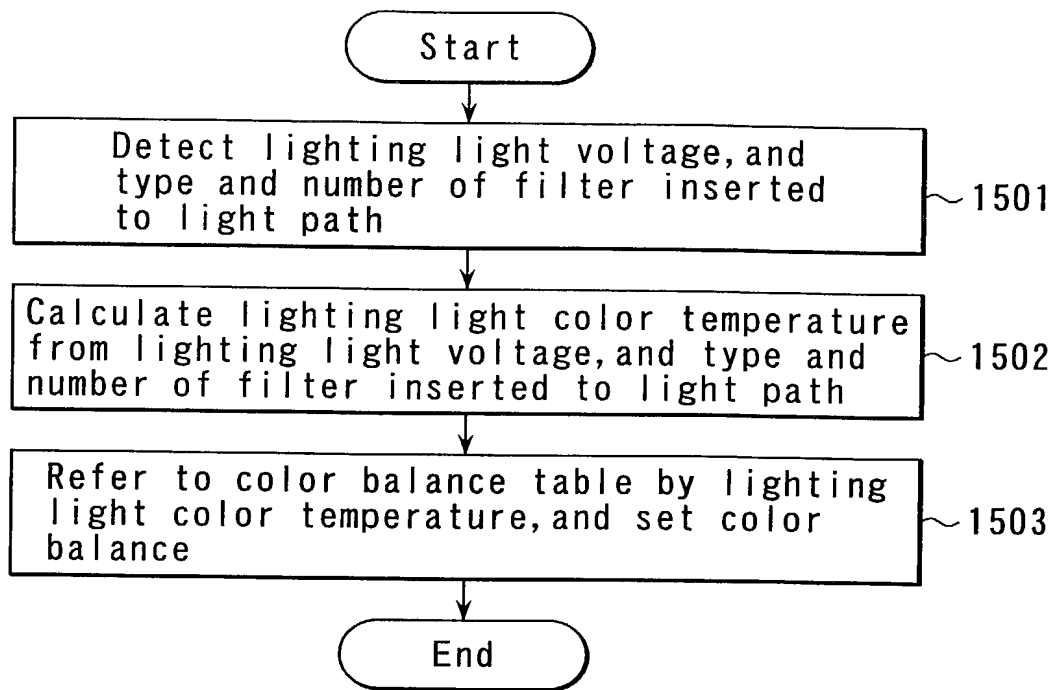


FIG. 13

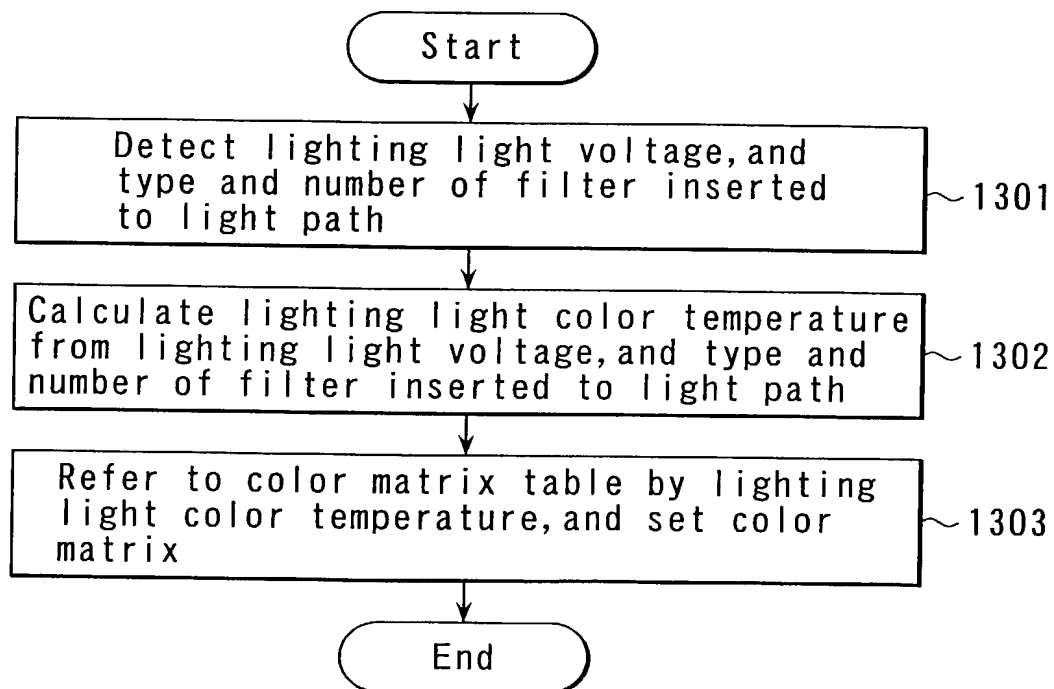


FIG. 14

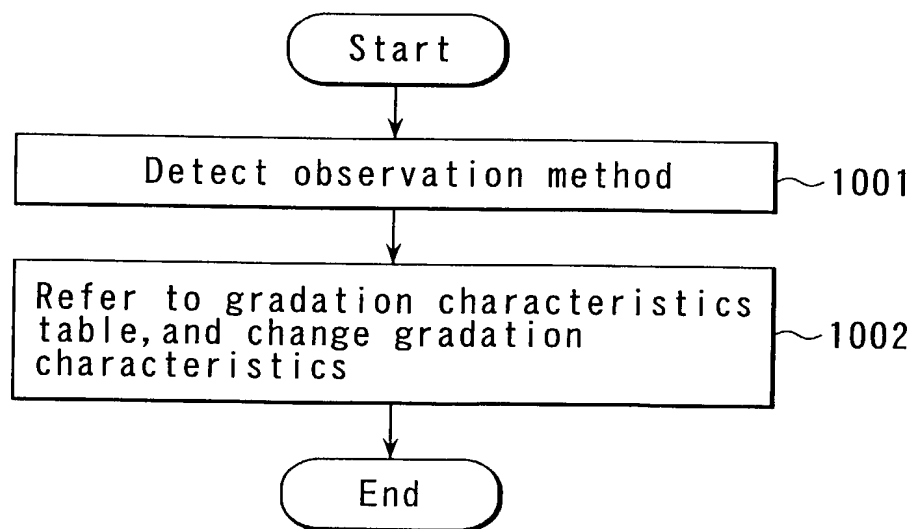
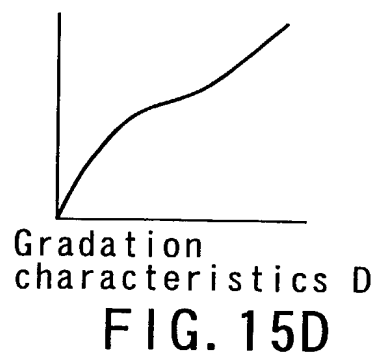
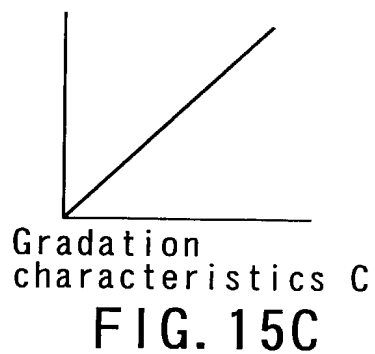
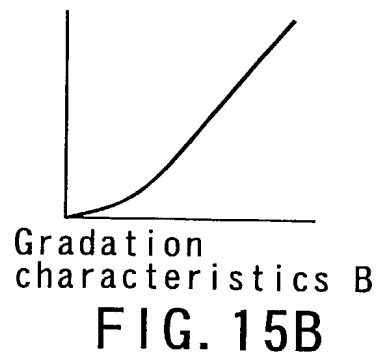
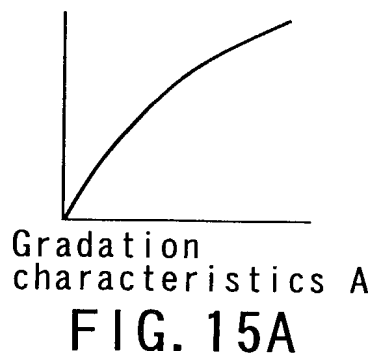


FIG. 16

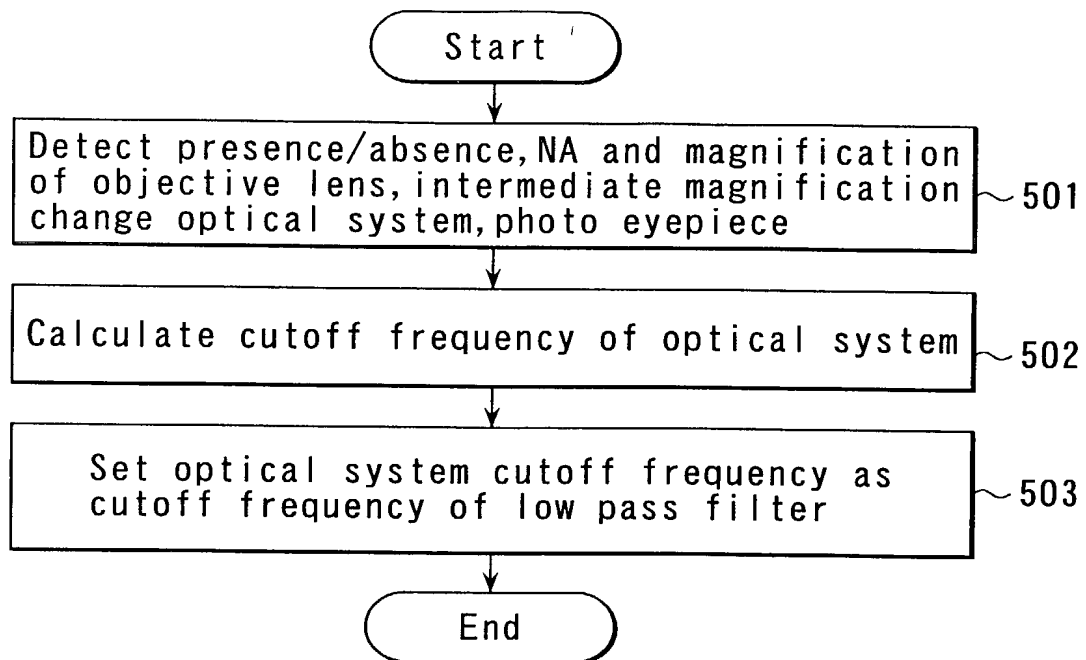


FIG. 17

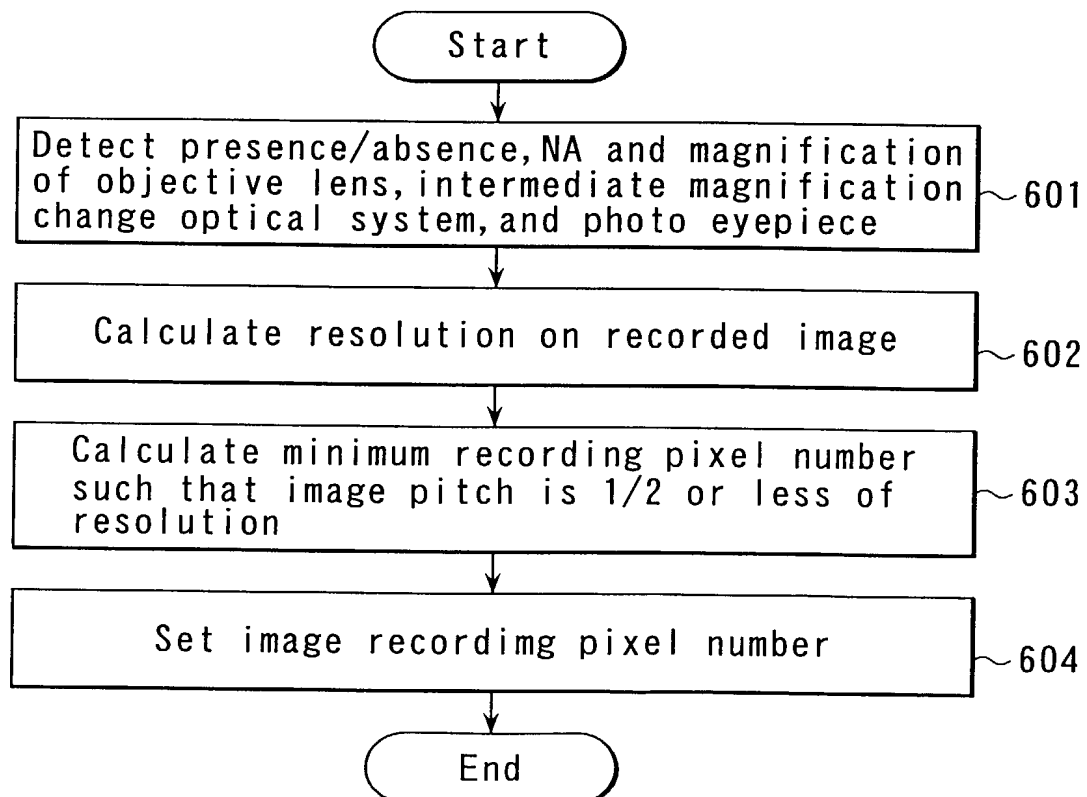


FIG. 19

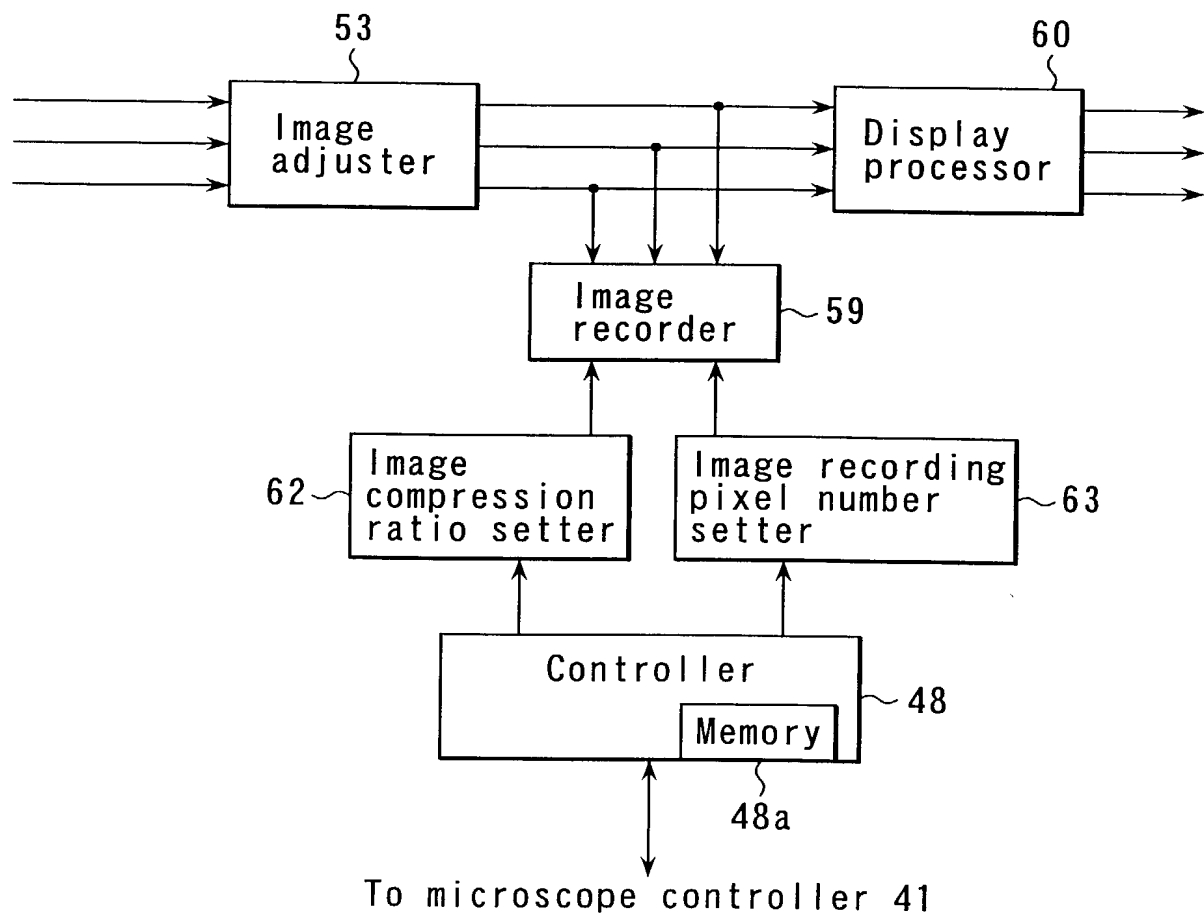


FIG. 18

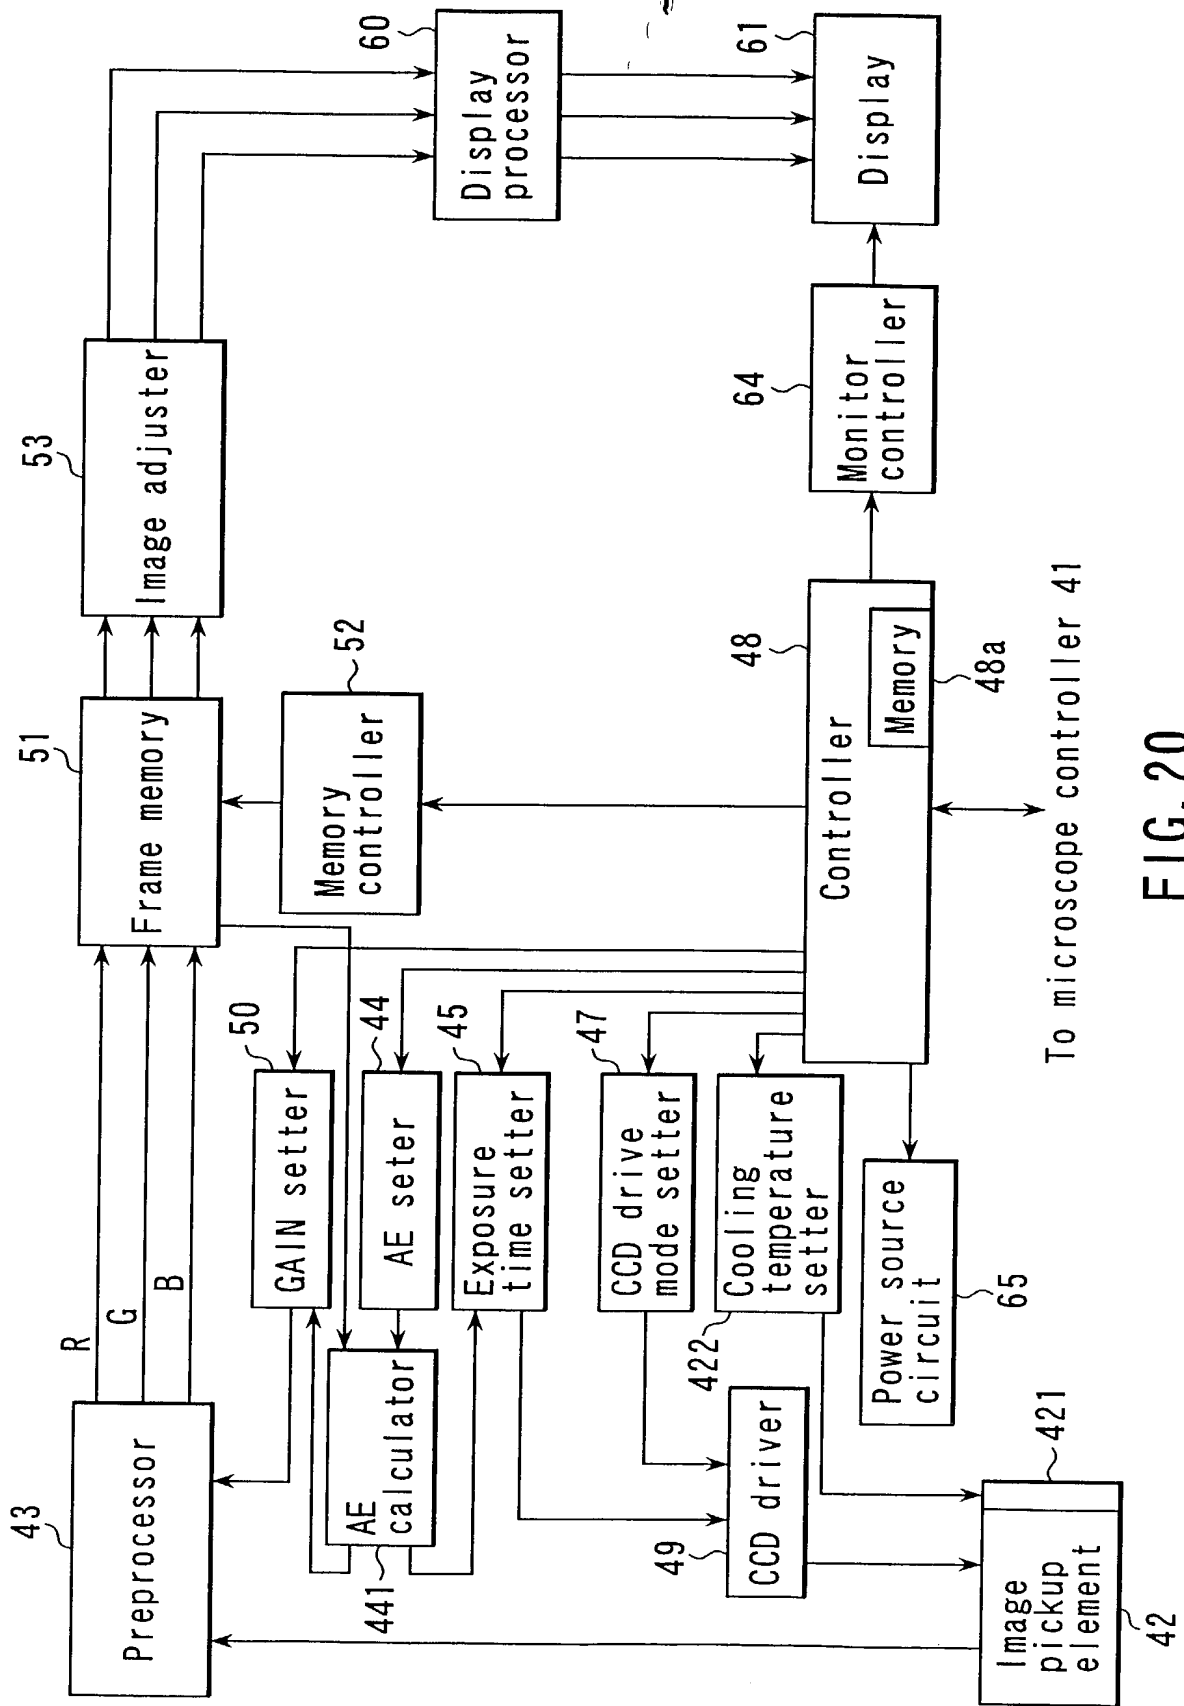


FIG. 20